
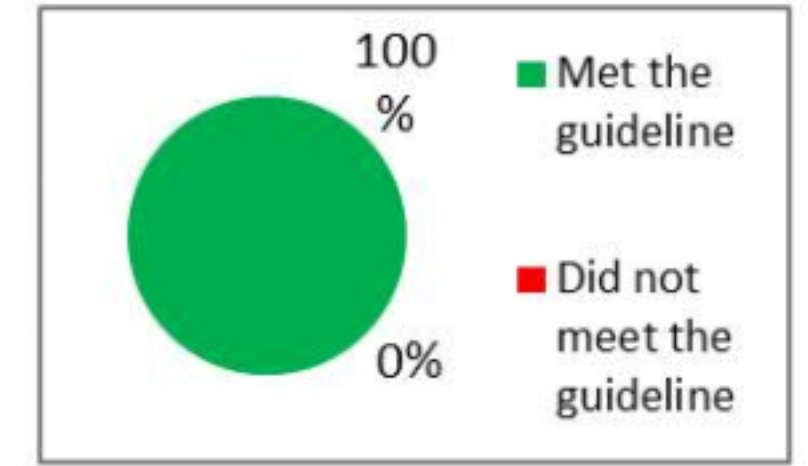


*Escuminac Swim Watch Results 2002 - 2019

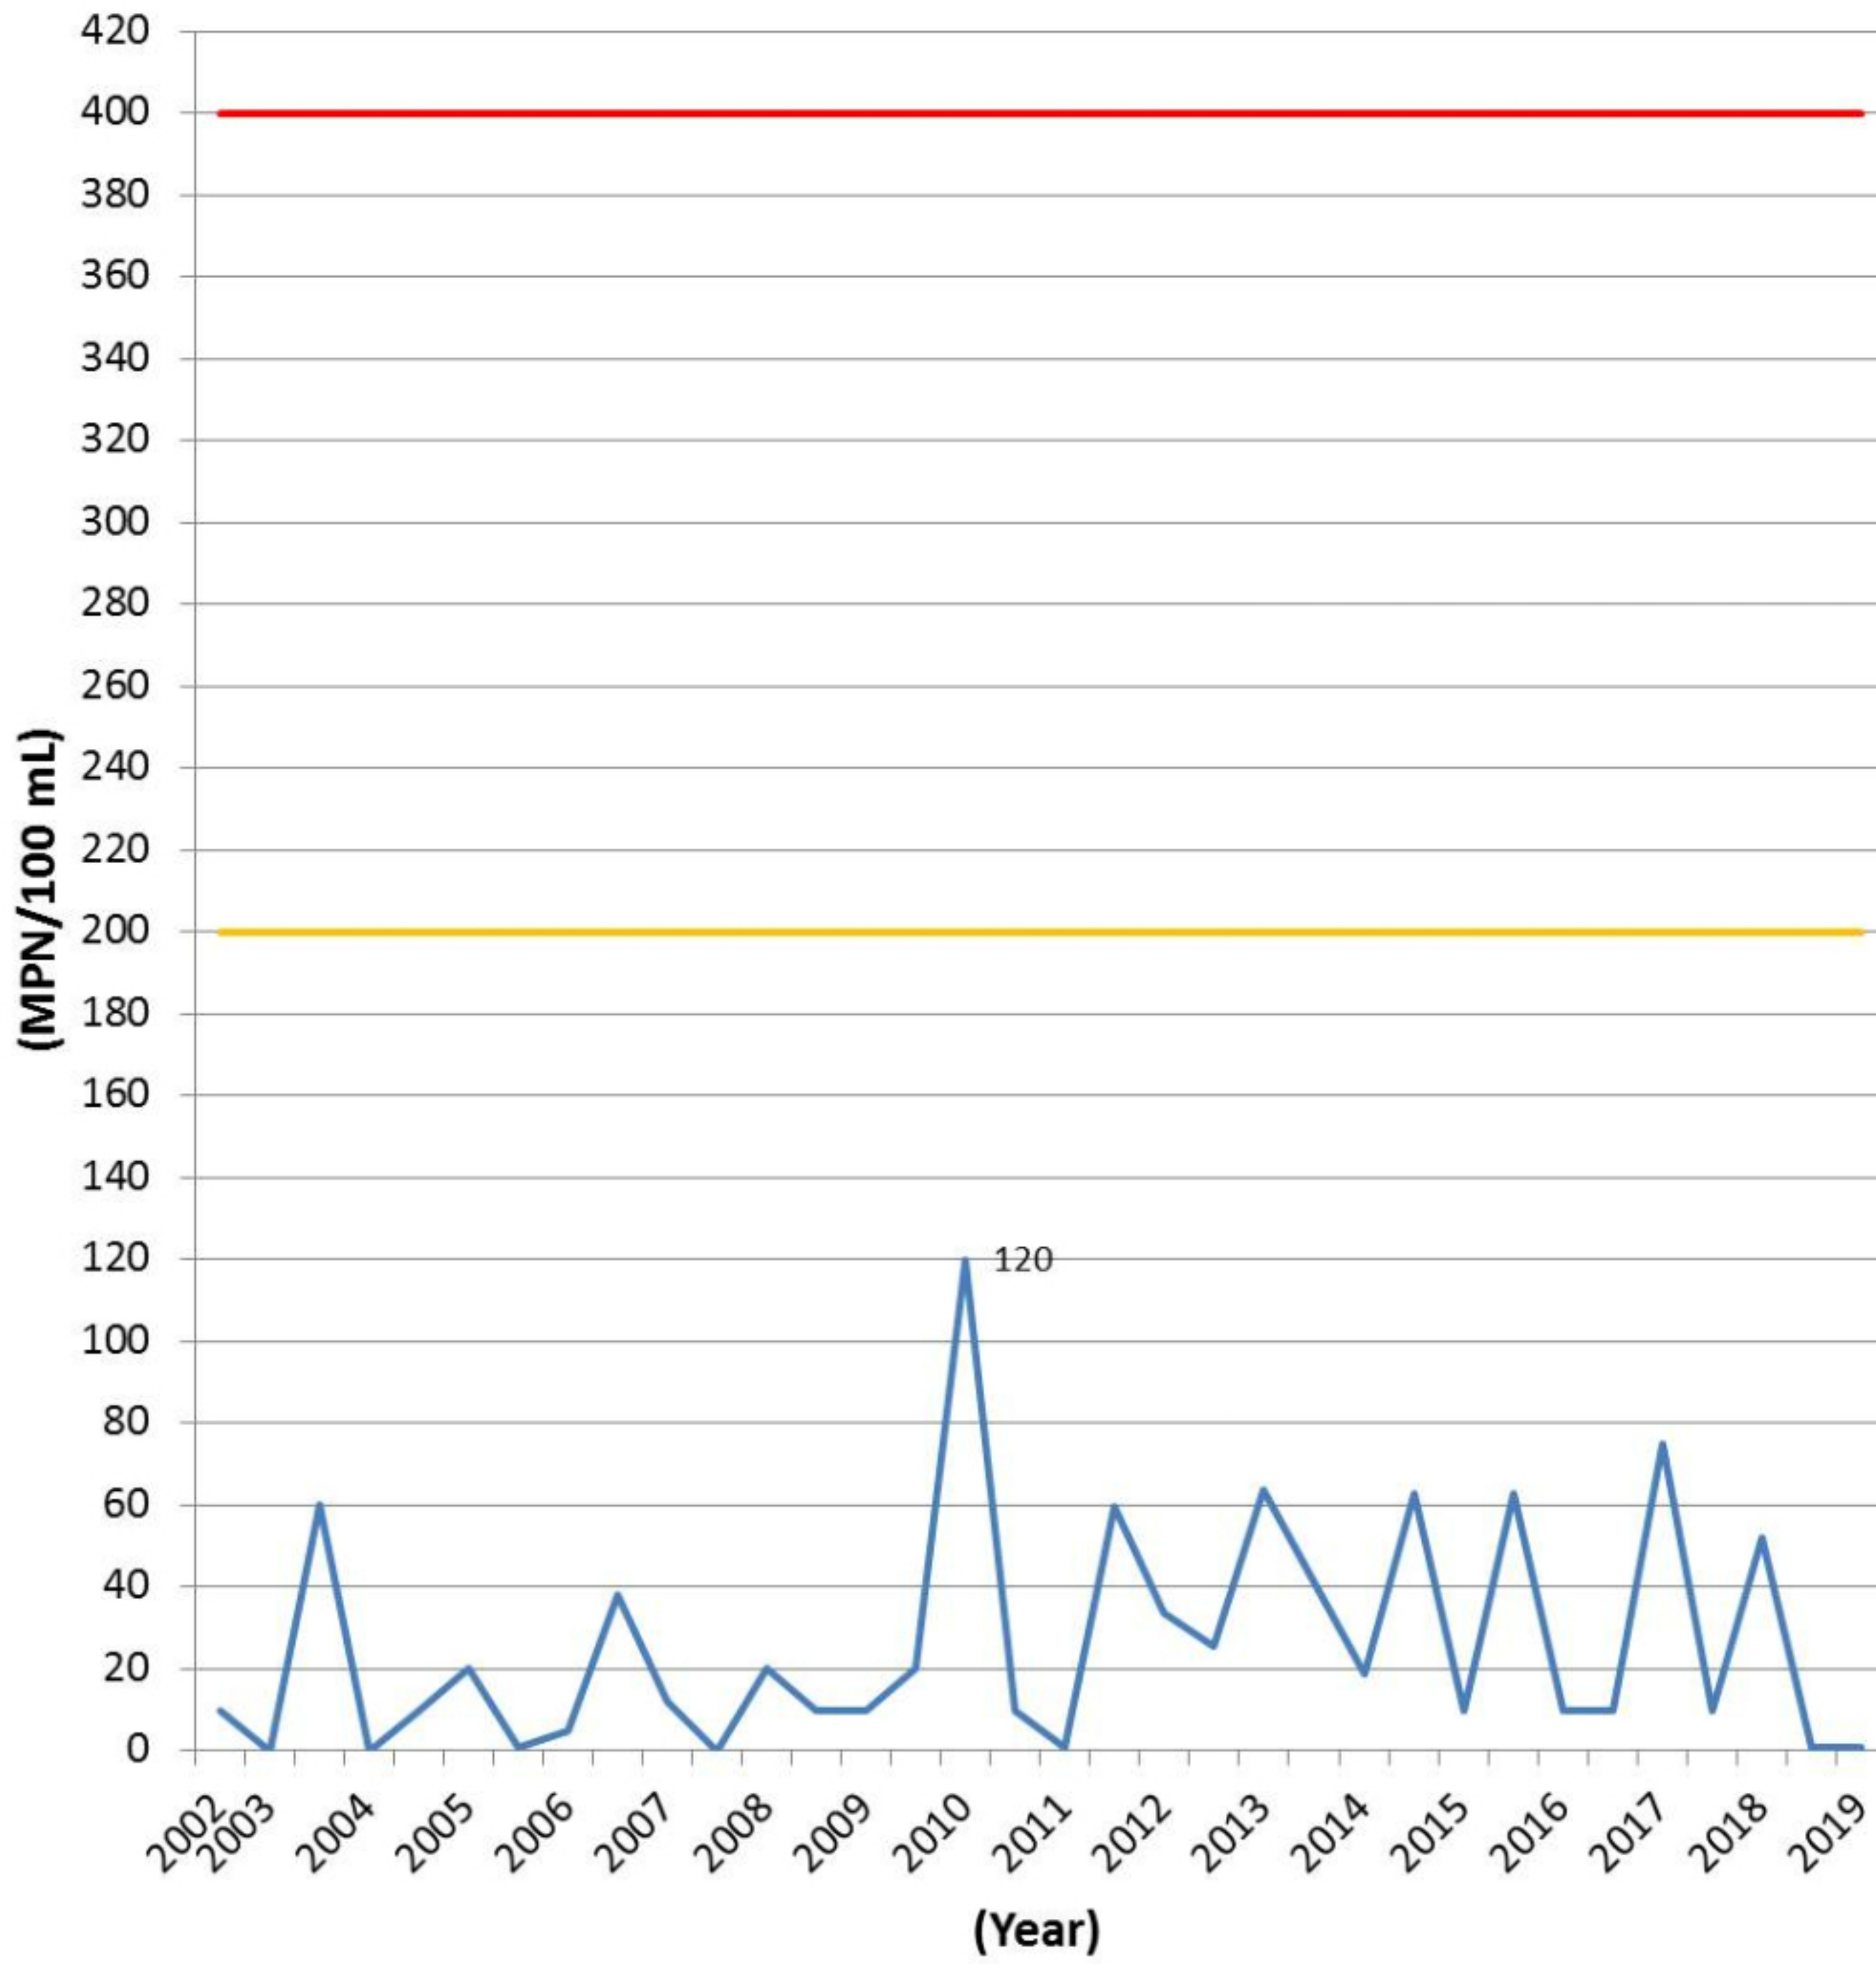

- Single-sample Maximum (400 E. coli/100 mL)
- Geometric Mean Concentration (200 E. coli/100 mL)
- E.coli Analytical Result

Based on 34 samples
All 34 samples meet the guideline

* These results are not from an accredited laboratory